

SLICE-DCC Dual-Channel Current Controller

Model No. SLICE-DCC

Document Revision: 1

Document Last Updated on 2025/07/01 01:05

Please read [Limited Warranty](#) and [General Warnings and Cautions](#) prior to operating the SLICE-DCC.

Links

Click here for the [main manuals page](#).

Click here for the [SLICE-DCC Serial API Guide](#).

Click here for the [SLICE-DCC web page](#).

Click here for the [Github page for SLICE-DCC GUI](#)

Click here for the [Github page for SLICE-DCC firmware revisions](#)

Please check back for added functionality. Contact [sales \[at\] vescent \[dot\] com](mailto:sales@vescent.com) for questions and corrections, or to request added functionality.

List of Warning Symbols

	Warning. Pay special attention to procedures and notes. If procedure is not followed carefully, damage to the SLICE-DCC or devices connected to it may occur.
	Potential for electrical shock hazard.

The SLICE-DCC Current Controller is intended for driving laser diodes. When using lasers particular care must be given to avoid exposure hazards.



Description

The SLICE-DCC is a low-noise, economical current controller (see [figure 1](#)). It serves as a low-noise current source providing up to 2 A. It is configured to work with a grounded cathode in either a constant current or a constant power mode.

Fig. 1: The SLICE-DCC



Model	Current Rating
SLICE-DCC-200	200 mA
SLICE-DCC-500	500 mA
SLICE-DCC-1000	1 A
SLICE-DCC-2000	2 A

Tab. 1: Available SLICE-DCC models

Purchase Includes

- SLICE-DCC dual-channel Current Controller
- AC power cord with appropriate wall plug for you location (if known)
- One BNC grounding cap for door safety interlock
- Two keys for lock out
- Final Test Documentation

Absolute Maximum Ratings and Power Input

Note: All modules designed to be operated in a laboratory environment.

Parameter	Rating
Environmental Temperature	>15°C and <30°C
Environmental Humidity	<60%
Environmental Dew Points	<15°C
Maximum AC Line Input Current	2 A

Tab. 2: Absolute Maximum Ratings

The SLICE-DCC will accept input line voltages within the ranges shown in [table 3](#).

Parameter	Value	Units
Input Line Voltage	100-240	VAC
Frequency	50-60	Hz
Phase	1 phase	
User-serviceable fuse ¹⁾	HBC 2.0 A 250V	

Tab. 3: Input Voltage Specifications

Proper Usage

	If this instrument is used in a manner not specified by the manufacturer in this manual or other relevant literature, protection provided by the instrument may be impaired.
	Use caution when connecting the SLICE-DCC to your diode. Diode lasers are static sensitive and can be damaged from static build up. Make sure to discharge any charge built up on your skin or clothes by using a grounding strap while making connections.

The SLICE-DCC is designed to drive, among other devices, laser diodes, quantum cascade lasers, and semiconductor amplifiers. In order to be in US FDA compliance for driving lasers:

- There is a 5 s delay between turning on the current and the current beginning to flow. During this period, a warning light will flash on the front panel of the SLICE-DCC.
- The key switch on the rear panel must be in the on position (where you cannot remove the key).
- The interlock connector on the rear panel must be shorted either with the 50 Ω terminator supplied with the device or via an external circuit including, for instance, a (closed) entranceway.



If either the key switch is deactivated or the interlock is opened while the system is operating, the SLICE-DCC will stop delivering current and the Enable window will flash red with INTERLOCK displayed ([figure 36](#)). In order to resume normal operation, interlocks must be restored to their operational state and the window must be touched to reset the tripped interlock.

Proper use of the interlocks requires that the door interlock circuit does not connect to ground as this may also engage the interlock warning.





Always power down the SLICE-DCC completely before making connections to a laser. Never connect or disconnect the SLICE-DCC to/from a laser with the SLICE-DCC energized.

As with any diode laser and controller, improper usage can cause irreparable damage to the diode.

Specifications

Performance ²⁾	
Parameter	Value
Channels	2
Control	Touch Screen, GUI, Serial commands
Operation Modes	Constant Current Constant Power
Maximum Current per Channel	200 mA 500 mA 1,000 A 2,000 mA
Current Noise ^{3) 4)}	1.5 μ A 4 μ A 10 μ A 15 μ A
Current Modulation Input Impedance Rear Front	>20 k Ω 50 Ω or 1 M Ω
Modulation Bandwidth ^{5) 6)}	DC to >1 MHz
Modulation Input Range	± 10 V
Modulation Depth SLICE-DCC-200 SLICE-DCC-500 SLICE-DCC-1000 SLICE-DCC-2000	± 10 mA ± 25 mA ± 50 mA ± 50 mA
Modulation Transfer Function SLICE-DCC-200 SLICE-DCC-500 SLICE-DCC-1000 SLICE-DCC-2000	1 mA/V 2.5 mA/V 5 mA/V 5 mA/V
Current Resolution SLICE-DCC-200 SLICE-DCC-500 SLICE-DCC-1000 SLICE-DCC-2000	10 μ A 10 μ A 20 μ A 100 μ A
Drift	<25 μ A/ $^{\circ}$ C
Power Stability ⁷⁾	0.1% rms ⁸⁾
Monitor Photodiode Input Current Range	± 5 mA

Maximum Compliance Voltage	12 V
Triggering	TTL

Tab. 4: Specifications of SLICE-DCC

Front Panel

An image of the front panel is shown in [figure 2](#). The functions and connections are as follows:

1. Parameter input adjustment knobs
2. Control signal inputs
3. Signal monitor outputs
4. CH status (Constant Current or Constant Power)
5. Current enable (CH1 is ON, CH 2 is off)
6. Current or Power set point
7. Optical Power or Diode Voltage display

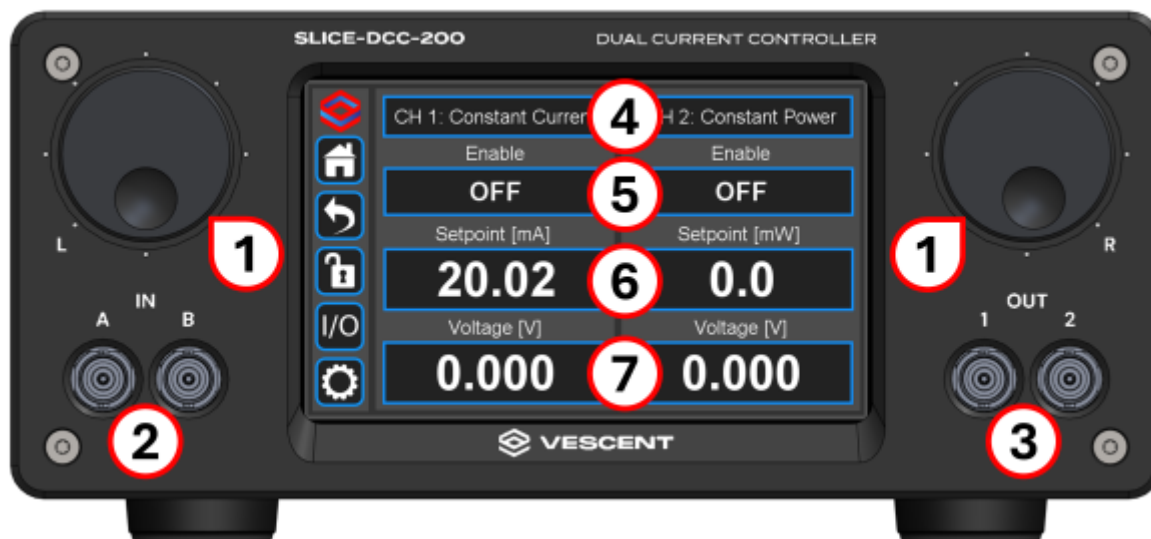


Fig. 2: Front of SLICE-DCC

Rear Panel

An image of the rear panel is shown in [figure 3](#). The functions and connections are as follows:

1. Main On/Off power switch
2. User-serviceable fuse: High breaking capacity 5mm x 20mm fuse rated to 250 V and 2A - Output trigger (BNC)
3. AC line power in⁹⁾
4. Input trigger (BNC)
5. USB port (Type B)
6. Interlock key receptacle
7. Door interlock
8. CH 2 Current output
9. [CH 2 Modulation input](#)

10. CH 2 Photodiode input

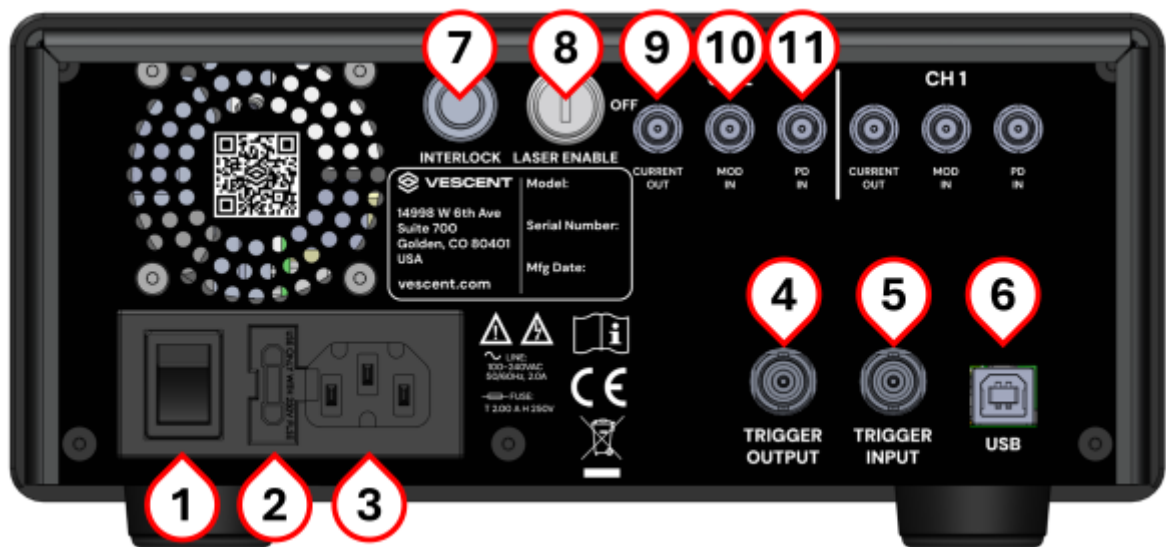


Fig. 3: View of rear of SLICE-DCC

Getting Familiar with the SLICE-DCC

Screen Navigation

The touch screen interface and the Host GUI operate in a substantially similar way, except touch is substituted for a click in the touch screen interface.

When presented with a given view, it is possible to select the functionality or edit the values in a field bordered in blue. When a particular field is actively being edited, its border will change to yellow. The Home Screen of the SLICE-DCC is shown in figure 4 and is reached by clicking the home button (figure 5) in the upper left corner of the touch screen. From the Home screen, summary control over the two channels is possible, including setting I_{set} or P_{set} . From the Home screen, you can edit the control parameters for each channel.

In general, the status displayed in an editable field is the current status (not the result of touching the button). Touch the field to select a new value/status. For instance, in figure 4 both channels are in stand by. Touching the OFF button will initiate current delivery to the given channel.

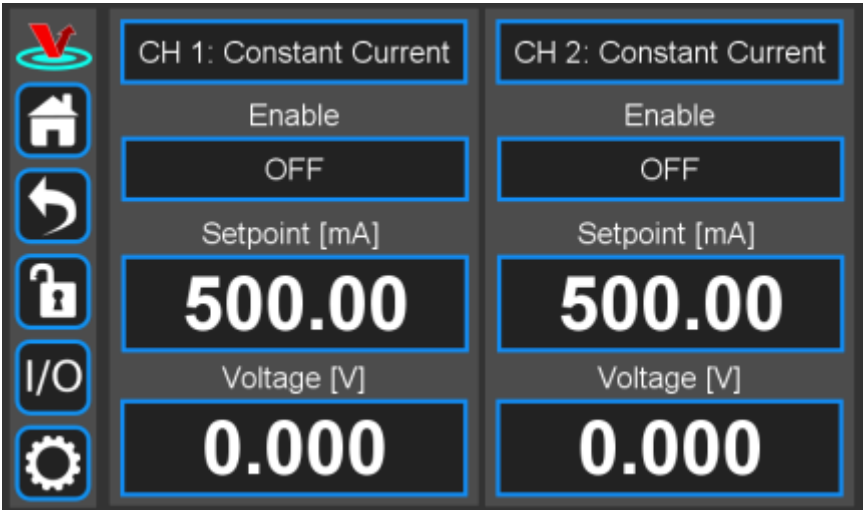


Fig. 4: Home screen of SLICE-DCC

Control Bar

On the left edge of the screen is the Control Bar. At any given time, these buttons will have the following effect.

Home Button



Fig. 5: Home button Returns to [Home screen](#) (figure 4).

Back Button



Fig. 6: Back button Returns to previous screen. Changes will be lost if not accepted before using the Back button.

Lock Button



Fig. 7: Lock button (shown in unlocked mode) Locks out further modification of parameters. Touch to lock or unlock parameter entry. When in lock mode, it is still possible to toggle the current on and off, but it will not be possible to change the set point or other operation parameters.

I/O Button



Fig. 8: I/O button Enters the screen for programming the [front-panel I/O](#).

System Settings Button



Fig. 9: System settings button Enters screen for [system control settings](#) (brightness, volume, etc.).

Entering Values

In most instances, there are two methods for entering parameter values: the physical rotary knobs on the front panel and the pop-up keypad on the touch screen. When using the knobs to change the value of a parameter, changes take effect immediately. When using the keypad, changes do not take effect until the enter key is touched.



In order to afford maximum resolution, the least significant digit will not necessarily change to precisely your target value and will be coerced to the nearest acceptable value, which is limited by the digitization scheme for the set point. For instance, you may select a set point current of 151.13 mA, but the closest allowed digitized value may be 151.14 mA.

Rotary Knobs

If you touch an editable field for a brief moment, the border of the field will change from [blue](#) to [yellow](#) and a cursor will appear under one of the digits of the parameter value ([figure 10](#)). By turning the right knob, it is possible to increase (cw) or decrease (ccw) the value of the underlined digit. Turning the left knob will change which digit is editable (cw to move to the right and ccw to move to the left). Changes made with the rotary knobs take effect immediately.

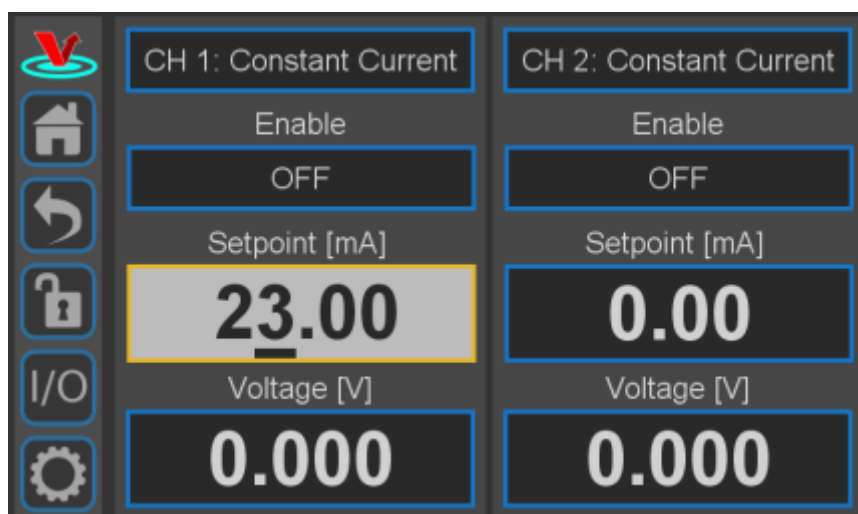


Fig. 10: Knob adjustment of Current set point for CH 1

Keypad

If you touch and hold an editable field such as the current set point, a numeric keypad will appear as seen in figure 11. You can enter in the full value of the desired parameter with this keypad. Changes entered through the keypad are not enacted until the Enter key is touched.

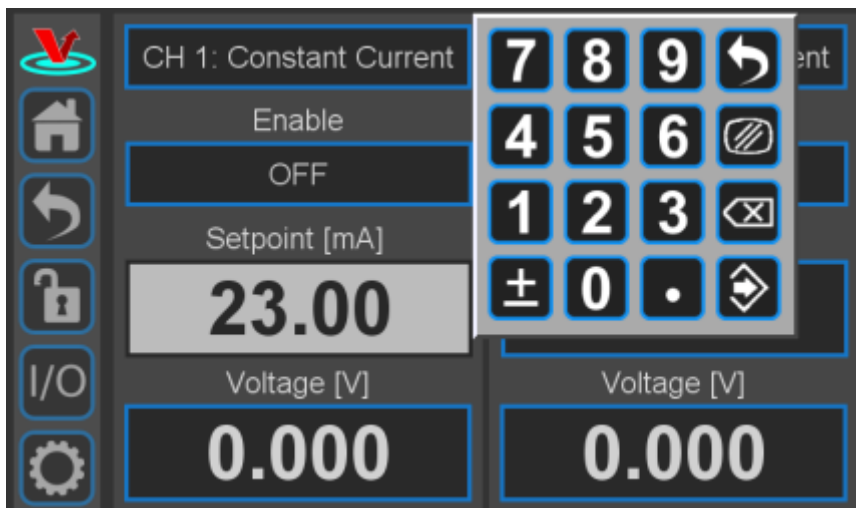


Fig. 11: Pop-up Keypad

The action initiated by each button of the keypad is described below.

Escape



Fig. 12: Escape button Exits keypad without accepting changes.

Clear



Fig. 13: Clear button Clears value in field being edited.

Delete



Fig. 14: Delete button Deletes last character entered.

Enter



Fig. 15: Enter button Accepts parameter edits and exits keypad.

Extendable Legs

The SLICE-DCC has four extendable legs (figure 16). Extending the front legs allows easy viewing from above (figure 1) and extending the rear legs (figure 17) allows easy viewing from below.



Fig. 16: Underside of SLICE-DCC



Fig. 17: Side view of SLICE-DCC configured for viewing from below

SLICE-DCC Operation

The Home screen displays the status of both channels (figure 4). The data for each channel is arranged vertically. At a glance, for each channel, I_{set} and Compliance Voltage can be read. Touching the blue window labelled Voltage [V] will cause this window to toggle from displaying Compliance Voltage to displaying dissipated Power.

Laser and Photodiode Connections

Connection to Laser Diode

The SLICE-DCC requires that the cathode of the laser diode is at ground ([figure 18](#)). The anode is connected to the center conductor of the SMA connector on the rear of the SLICE-DCC and the cathode is connected to the sheath.

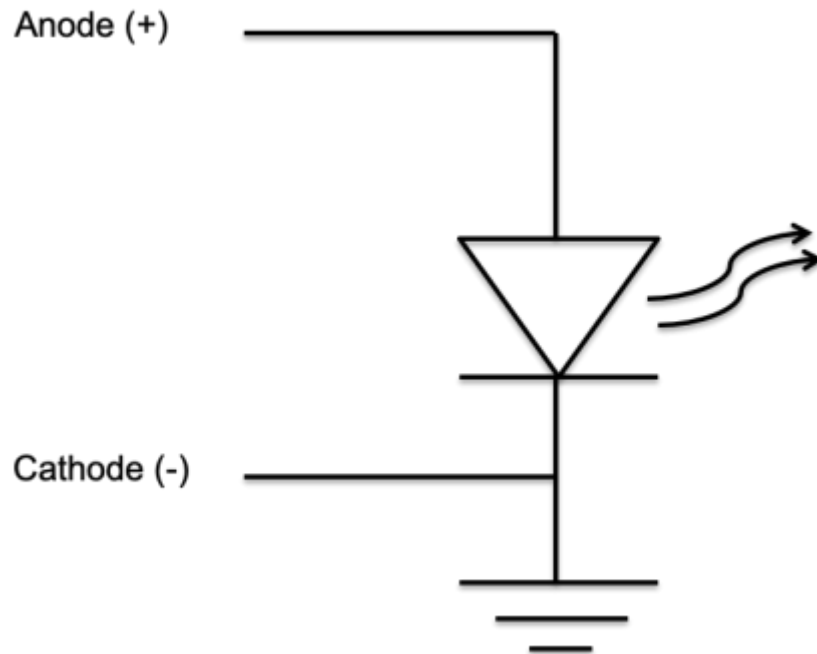


Fig. 18: Wiring configuration for laser diode

Connection to Monitor Photodiode

Either of the two configurations of the monitor photodiode seen in [figure 19](#) will work for the signal proportional to the laser diode power for operating in Constant Power mode. Depending on how you have completed the monitor photodiode circuit, you may have to adjust the [sign of the Constant Power feedback loop](#).

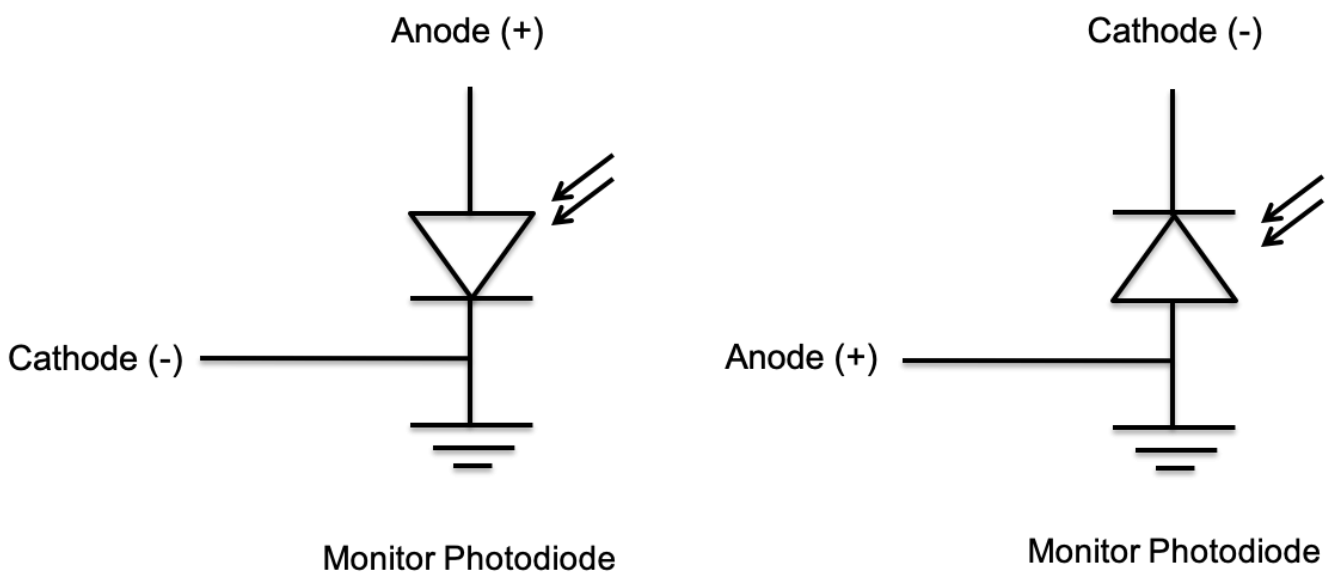


Fig. 19: Wiring configurations for monitor photodiode

Setting the Operation Mode

The SLICE-DCC has two operation modes: Constant Current and Constant Power. The operation mode, as with most other operating parameters can be set independently for each channel. To toggle between Constant Current and Constant Power modes, from the Home screen, touch the window labelled either CH X Constant Current or CH X Constant Power. If the channel is in Constant Current Mode, you will be presented with the window seen in figure 20.

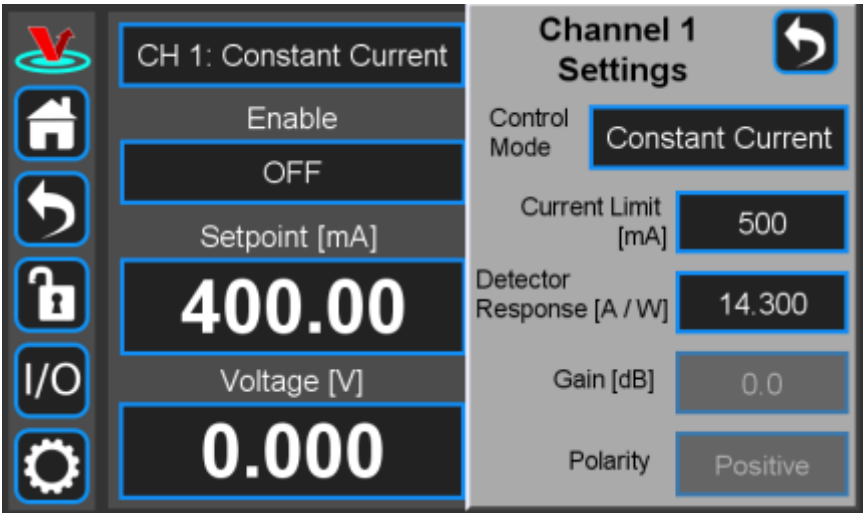


Fig. 20: Setting Maximum Current

If the channel is in Constant Power mode, you will be presented with the window seen in figure 21.

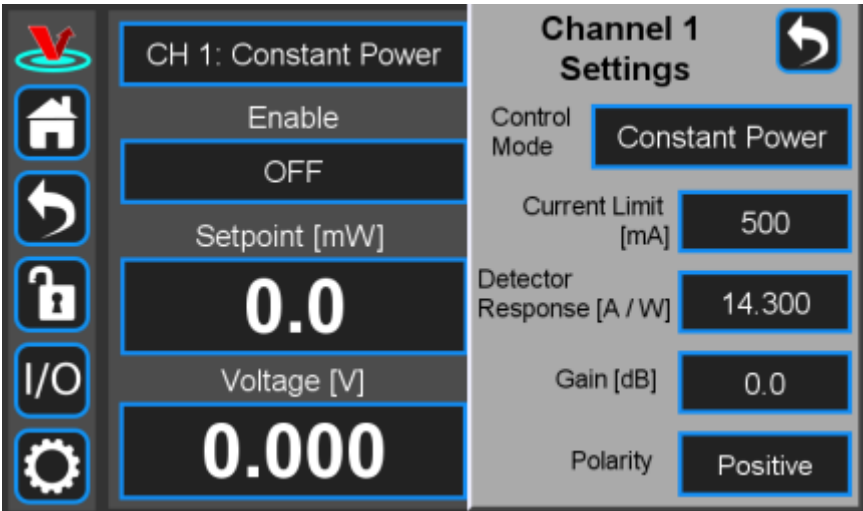


Fig. 21: Selecting Constant Power mode parameters

Touching the Window labeled Control Mode will allow you to toggle the channel back & forth between Constant Current and Constant Power modes as seen in figure 22.

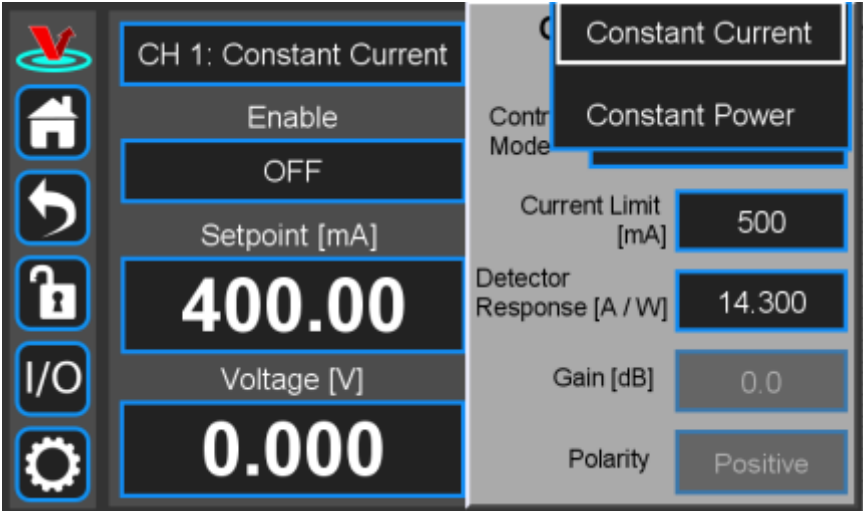


Fig. 22: Constant Current or Constant Power

Setting the Current Limit

The user can set a maximum deliverable current so as not to exceed the rated maximum for their device. From the Home screen, touch the window labelled either CH X Constant Current or CH X Constant Power. Depending on the operation mode, you will be presented with either figure 20 or figure 21. Touch the Current Limit window and enter the maximum allowed current (in mA) as in figure 23.

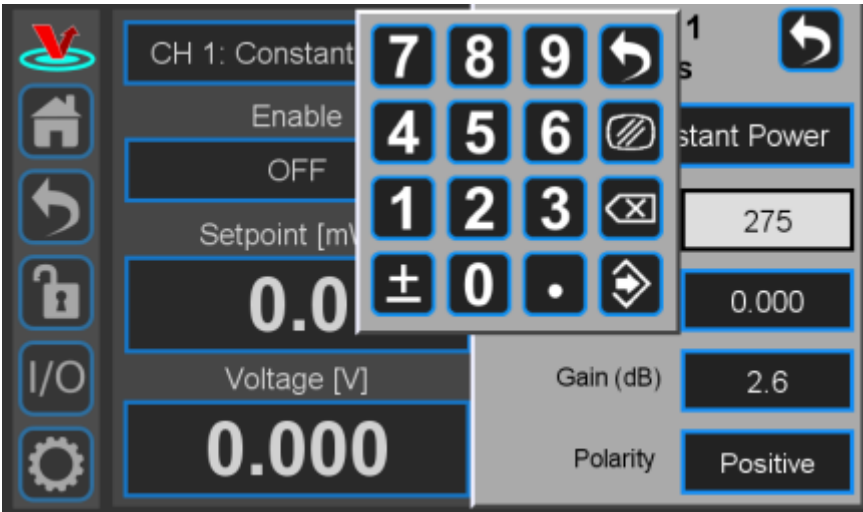


Fig. 23: Set Current Maximum

Setting the Operating Current in Constant Current Mode

In Constant Current mode a linear regulator minimizes current noise & fluctuations.

To set the current set point from the home screen, touch the Set point window for the desired channel. A long touch will cause a keypad to appear (figure 24). Enter desired value and touch the accept button.

A short touch will highlight the Setpoint window in yellow (figure 10). Use rotary knobs to select digit to edit (left knob) and value for digit (right knob).

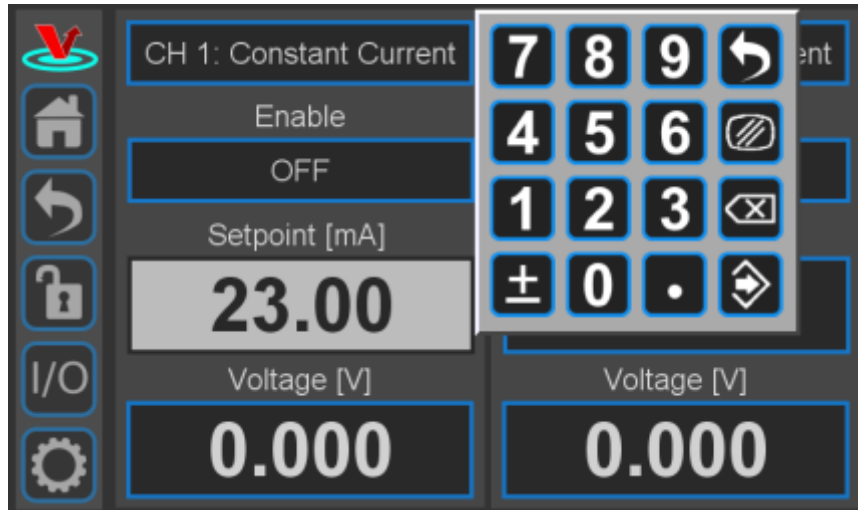


Fig. 24: Keypad adjustment of Current set point for CH 1

Setting the Operating Power in Constant Power Mode

To set the power set point in Constant Power Mode from the home screen, touch the window labelled Setpoint [mW] and enter the target power level ([figure 25](#)). If the window is labelled Set Point [mA], the device is in Constant Current mode and must first be [switched to Constant Power mode](#).

It is possible to adjust the Power Setpoint when the system is either ON or in Standby mode.

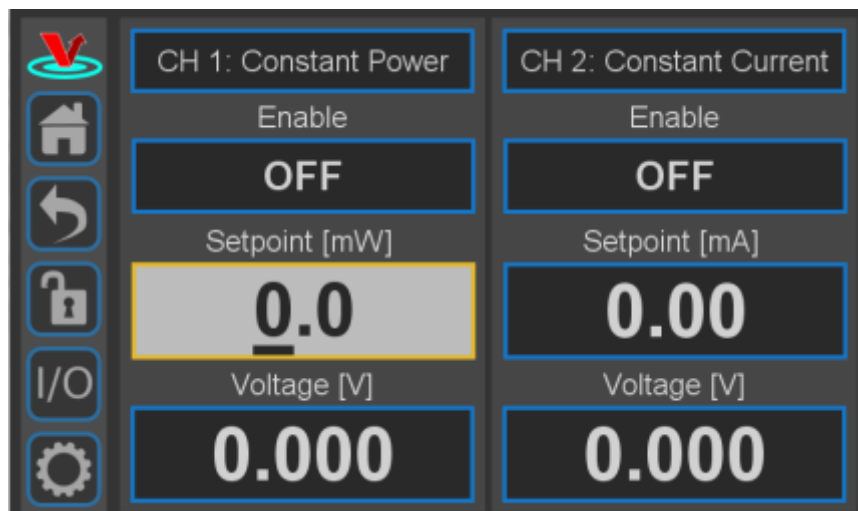


Fig. 25: Setting the power set point in Constant Power mode

Enabling Current

When the blue window labeled Enable reads OFF, the system is in standby mode and no current is delivered. Briefly touching this window will, after a 5 s pause during which a warning light will flash, cause current to begin to flow and the window will read ON.

Rear-Panel Modulation

On the rear panel of the SLICE-DCC is an SMA input for servoing or modulating the current output. ([figure 3](#), item 9). The input range is ± 10 V. The transfer function for this input depends on the


current capacity (see [table 4](#)). The 3-dB bandwidth of this modulation input is DC to 1 MHz.

It is also possible to introduce a modulation/control signal from the front-panel input BNC. Only one input port can be active at a time.

	Although there is protection circuitry to reduce reverse biasing the diode, negative voltages as high as -0.5 V can be applied. It is not advisable to modulate under conditions where negative voltage would be applied. Avoid low current set points with large-amplitude modulation.
	Make sure that the modulation input cannot drive the current above the maximum rated current for your device by setting the Current Limit appropriately .

Constant Power Mode

In Constant Power mode, the SLICE-DCC accepts a current input signal from the output of a photodiode (often internally mounted with the diode laser). This signal is conditioned by a trans-impedance amplifier and used as an error signal. It is further processed by a loop filter to provide a correction signal to the current to maintain constant power.

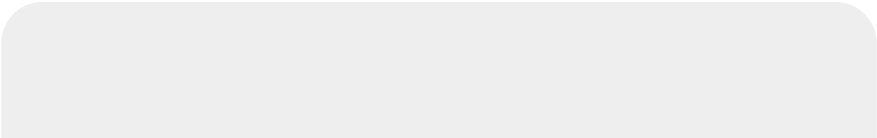



1. Connect the output of the monitor photodiode to the CH X Photodiode Input connector (labelled "10" in [the back-panel image](#)) on the back of the SLICE-DCC.

In order for Constant Power mode to operate correctly, the user must set three control parameters: the responsivity of the monitor photodiode, the gain of the loop filter, and the polarity of the photodiode response. Before setting these control parameters. First [set the SLICE-DCC in Constant Power mode](#) and [set the Power Setpoint](#). From the home screen, enter the CH X Settings screen by tapping the window labelled CH X: Constant Power. Enter values for Detector Response, Gain, and monitor photodiode Polarity.

2. Enter the value of the detector response supplied in the documentation that came with your monitor photodiode. ([figure 26](#))

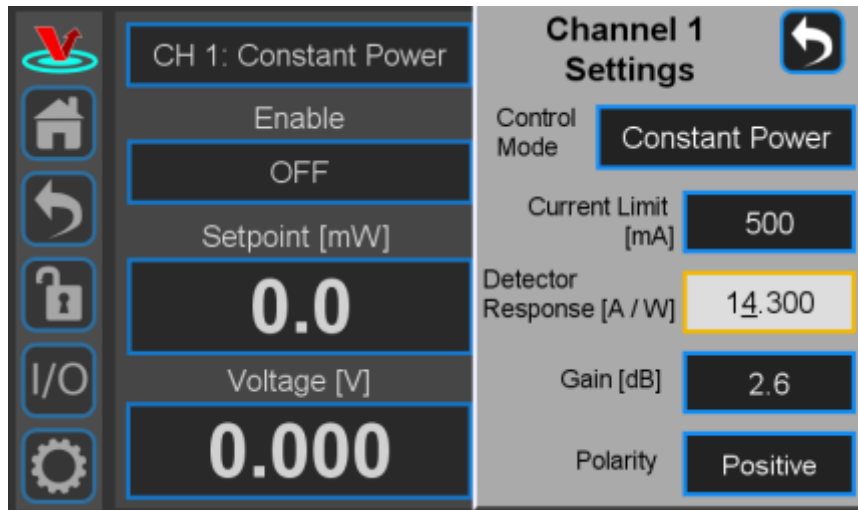


Fig. 26: Setting the detector response for Constant Power mode

3. Turn the Gain all the way to 0 (zero). Turn the system ON to deliver current to the diode. Slowly turn up the Gain until the power begins to oscillate (figure 27). (Hint; It is easiest to adjust the gain for this step via the knobs as opposed to through the keypad.) Turn down the Gain until oscillation stops.

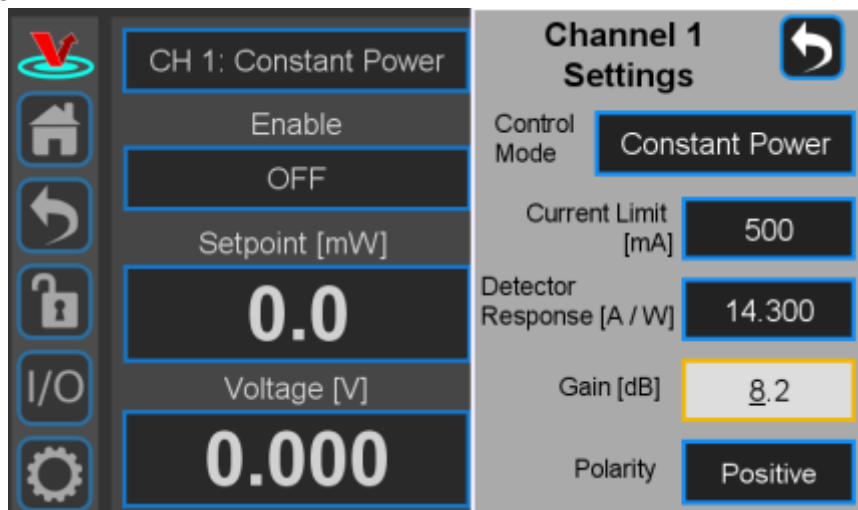


Fig. 27: Setting the Gain for Constant Power

4. If more Gain moves the power away from the set point, switch the polarity from Positive to Negative (or vice versa).

Programmable Input & Output

The SLICE-DCC has two programmable inputs (labelled A & B) and two programmable outputs (labelled 1 and 2) on the front panel. It also has a rear panel trigger input and trigger output. Touching the I/O icon on the control bar will open a screen similar to that seen in figure 28, From here, it is possible to assign control information input to the two inputs and system performance data to the two outputs,

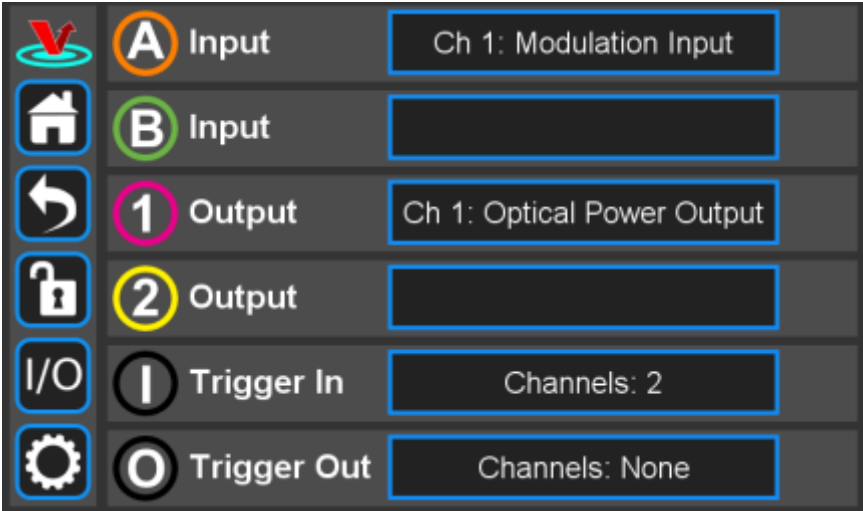


Fig. 28: I/O programming window

These front-panel inputs and outputs are mainly intended for monitoring the performance of the SLICE-DCC and as such have slower, noisier components than the rear-panel connections.

Programmable Input (Front-panel Modulation)

From [figure 28](#), if one touches either the A or B input window, the choices for input for that channel are presented ([figure 29](#)).

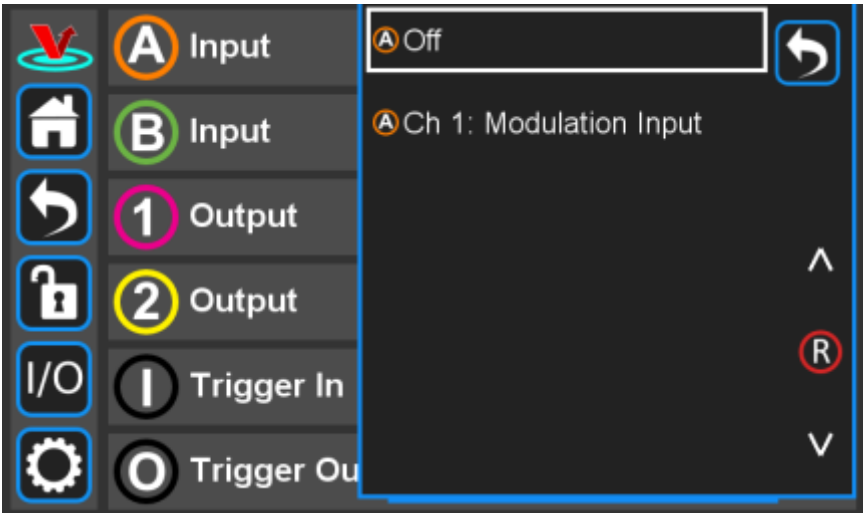


Fig. 29: Input choice for front-panel input

The only input option is a modulation signal. The SLICE-DCC can respond to a modulation or control signal over a bandwidth of DC to 1 MHz. Only one of the two modulation input ports (rear-panel SMA, [figure 3](#), item 9 or front-panel BNC, [figure 2](#), item 2) can be active at any given time. Activating the front-panel input via the screen in [figure 29](#) automatically disconnects the rear-panel input.

The depth and index of modulation varies depending on the current capacity of the particular SLICE-DCC unit. See [table 4](#).

Programmable Output

From [figure 28](#), if one touches either the 1 or 2 output window, the choices for output for that channel are presented ([figure 30](#)).

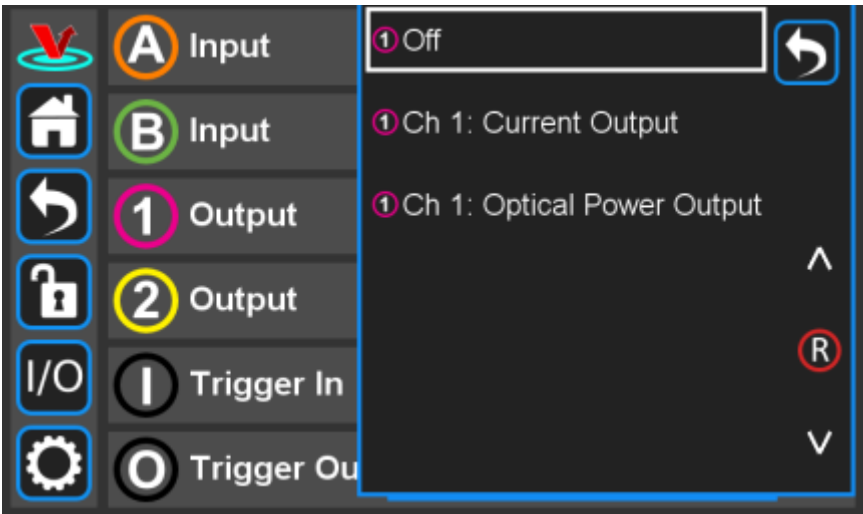


Fig. 30: Output choices for front-panel input

One can choose to monitor the current output and/or the optical power as measured at the photodiode input.

Triggering

External control of the SLICE-DCC is accomplished via a TTL trigger.¹⁰⁾ 0 to 0.8 V TTL is low and 2 to V_{cc} is TTL high.

Trigger Out

The Trigger Out on the back panel of the SLICE-DCC can be programmed to go high if an interlock (key or door) is opened. The screen shown in [figure 31](#) will be reached by touching I/O > Trigger Out. Checking the box will cause the Trigger Out to go high if either the door interlock or the key interlock is opened.

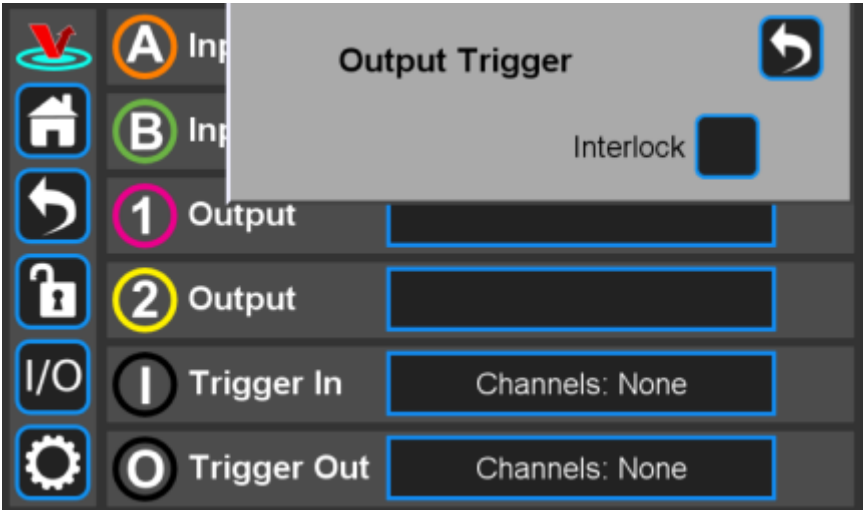


Fig. 31: Setting an output trigger

Trigger In

The input trigger can be used to turn on or off the current for either or both channels. From any screen, touch I/O > Trigger In. You will be presented with the window in [figure 32](#). Select which channels you wish to control with the incoming trigger. In [figure 33](#), current to CH 2 will be disabled if the Trigger In goes high.

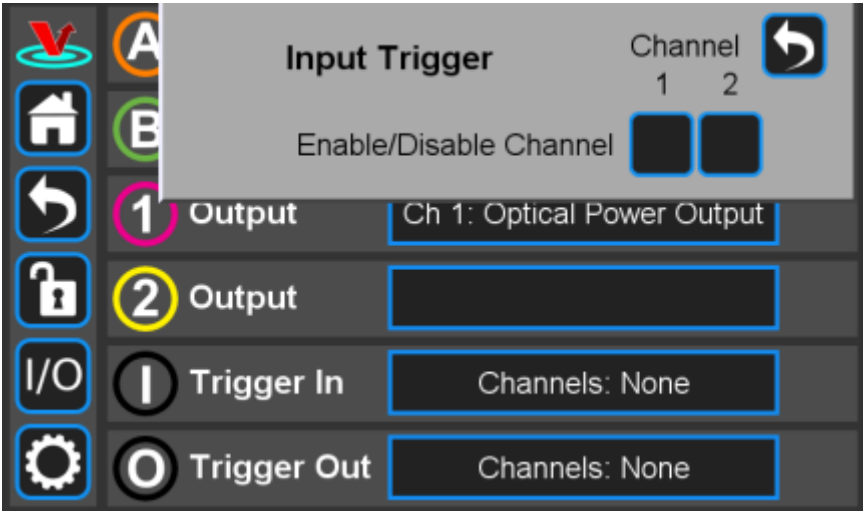


Fig. 32: Programming the rear-panel trigger in

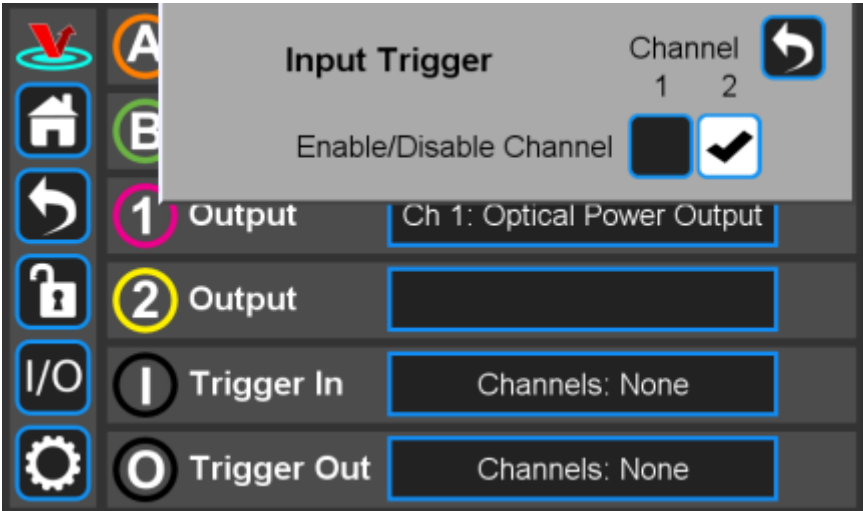


Fig. 33: CH 2 is controlled by input trigger

System Settings

Touching the [System Settings](#) button on the [Control Bar](#) ([figure 9](#)) will open the System Settings screen as seen in [figure 34](#).

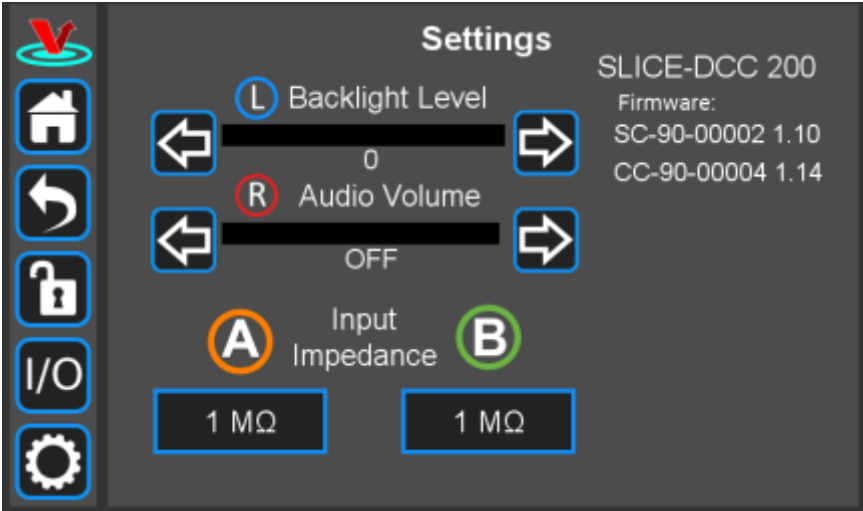


Fig. 34: User-programmable system settings

User Interface Appearance

From this screen, adjustments to the brightness of the screen and the volume of the audio feedback can be made.

Input Impedance

Change the input impedance of the two front-panel input ports. Select either 50 Ω or 1 MΩ.

SLICE Firmware

Current firmware versions are reported here.

Firmware	Version Level	Release Date
System Controller	1.24	23 May 2019
DCC	TBD	TBD

Tab. 5: Most recent firmware versions as of 6 June 2019

From time to time, Vescent will upgrade the firmware for controlling the SLICE-DCC. The procedure to upgrade the firmware is given [here](#).

Host GUI

If accessed through a PC Host GUI, the Settings screen (figure 35) also has the ability to assign the COM port for the device. If viewed through the GUI, there are no brightness or volume controls as these should be set on the PC directly.



Fig. 35: User-programmable system settings from host GUI

Error States

Interlock Open

If either the key switch is deactivated or the interlock is opened while the system is operating, the SLICE-DCC will stop delivering current and the Enable window will flash red with INTERLOCK displayed (figure 36). In order to resume normal operation, interlocks must be restored to their operational state and the window must be touched to reset the tripped interlock. This state may also activate if the Remote Interlock port becomes grounded.

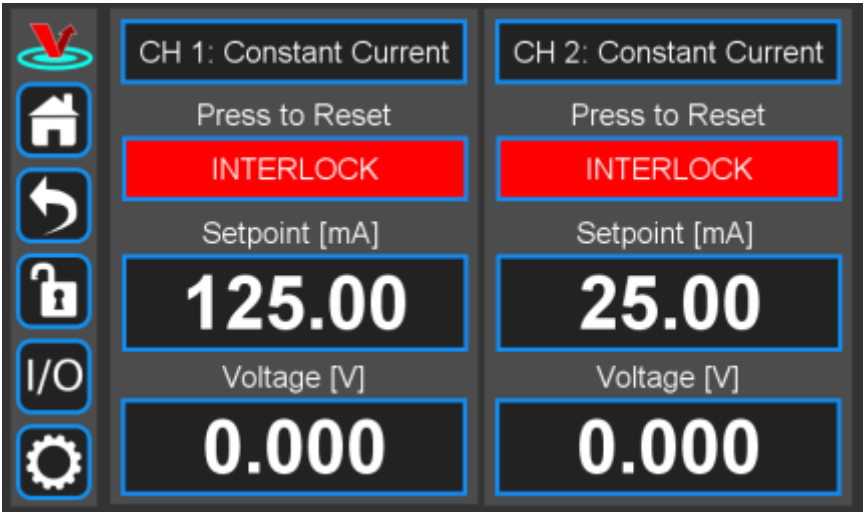


Fig. 36: Interlock Open state

Open Circuit

If the SLICE-DCC attempts to deliver current, but is unable to do so, it assumes an open circuit fault. The Enable window on the Home screen for that channel will flash red with the warning “Open Circuit/Over Voltage” (figure 37).

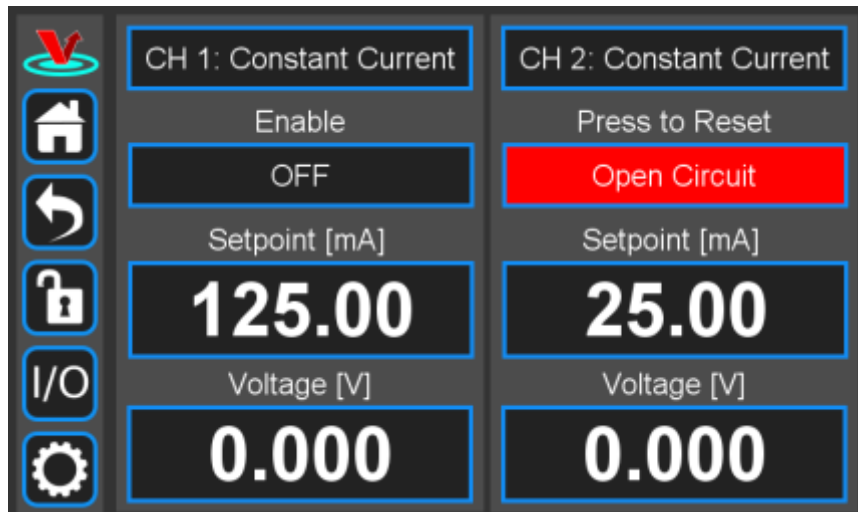


Fig. 37: Open Circuit detected

Using the Host GUI

It is possible to control the SLICE-DCC from a Windows®-based PC using the GUI written for this purpose. In order to use the GUI, you must first download the latest version, connect the PC to the SLICE-DCC, and assign a COM port to the SLICE-DCC. The following describes the steps involved.

1. Download and store the latest GUI executable from [the Vescent FTP site](#) (or request copy of executable GUI from [sales \[at\] vescent \[dot\] com](mailto:sales@vescent.com)).
2. Connect the SLICE-DCC to the PC using a USB type B cable.
3. Turn on the SLICE-DCC.
4. On the PC, double click on the SLICE-DCC GUI to start the GUI.
5. On your PC, go to Start > Control Panel > Device Manager > Ports
 1. Identify which COM Port is labeled “STMicroelectronics Virtual COM Port (COMXX)” or similar. Note the value of XX.



6. On the SLICE-DCC GUI, click on the Settings icon to get to the window shown in [figure 38](#).

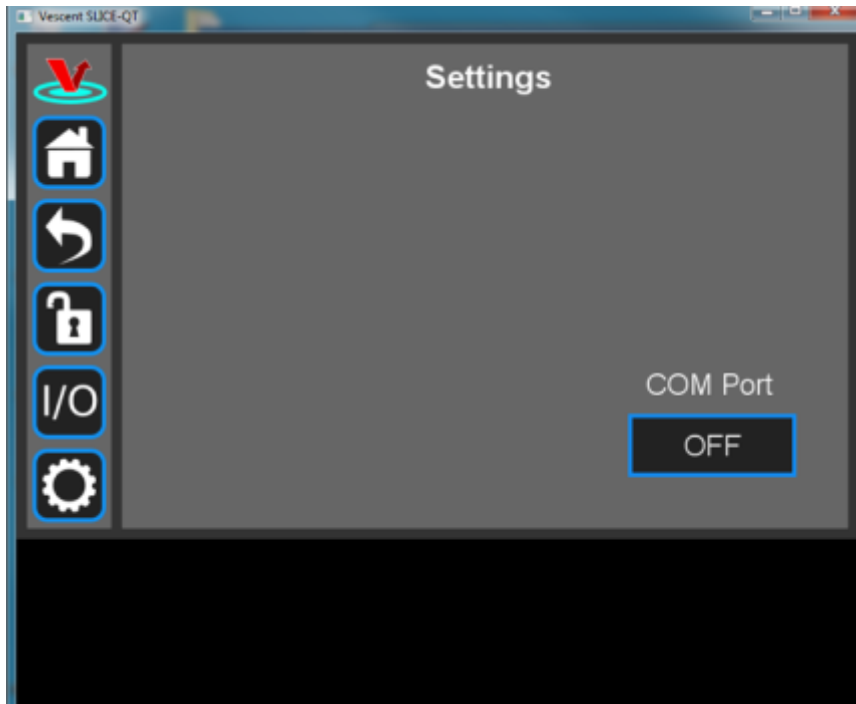


Fig. 38: Settings screen when viewed by GUI

7. Click on the OFF button below COM Port. You should see a menu similar to the one shown [figure 39](#). NOTE: The COM port numbers may differ from those shown below.

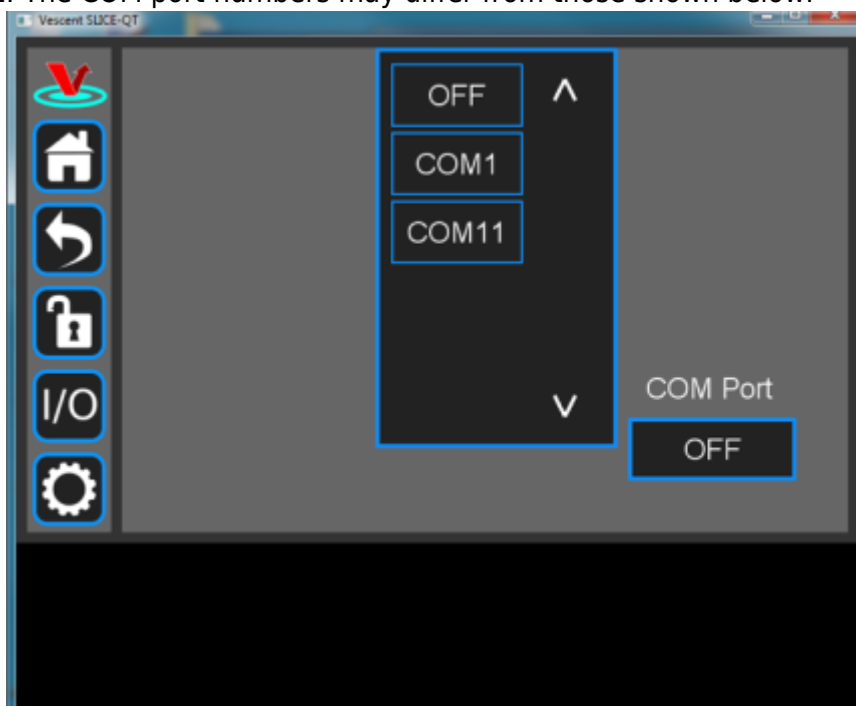


Fig. 39: COM port selection

8. Select the COM port identified in the step above (usually the last COM port in the list; COM11 in this example). The window in [figure 40](#) should appear if the connection is successful.

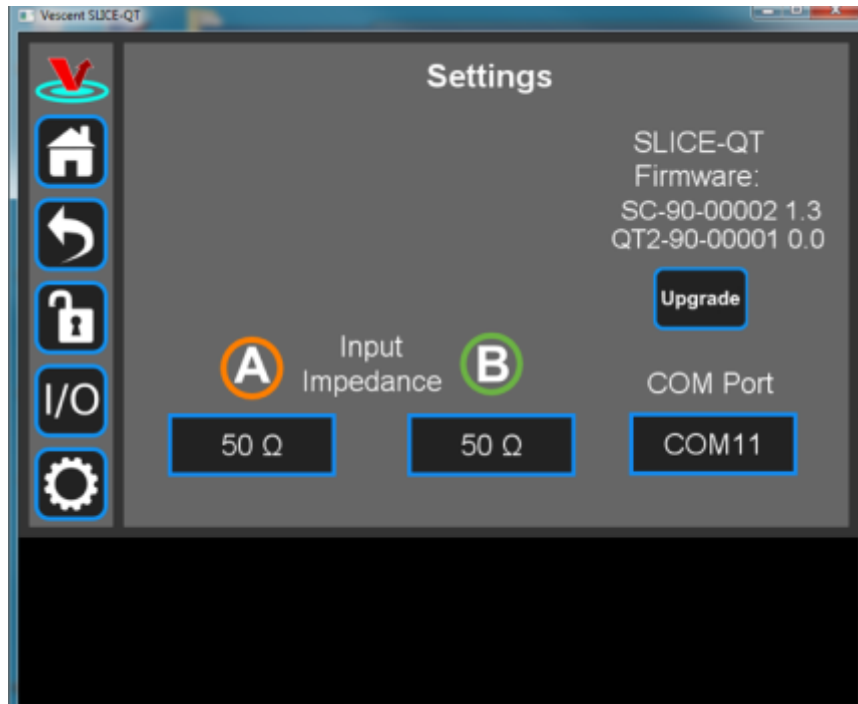


Fig. 40: Ready to upgrade

The GUI should now actively control the SLICE-DCC. You should only have to do the above steps once from a given PC. After assigning the COM port, the system will recognize the device in the future (unless you reassign the COM port to another device).

Firmware Update

From time to time, Vescent will upgrade the firmware for controlling the SLICE-DCC. The procedure to upgrade the firmware is given [here](#).

Serial API

It is possible to control the SLICE-DCC through serial commands. Click here to access the [SLICE-DCC Serial API Guide](#).



Upgrading the SLICE-DCC firmware is not always necessary to use the Serial API. Check your installed firmware version in the settings menu against the most recent firmware version given [here](#).

Please contact [sales \[at\] vescent \[dot\] com](mailto:sales@vescent.com) for information.

Maintenance

There are no user-serviceable parts inside this instrument. Refer all repairs to the manufacturer. Work

performed by persons not authorized by Vescent may void the warranty.

Warnings and Faults

Hardware Temperature Exceeded

Displayed when hardware temperature exceeds a safe limit for an individual channel. Turn off the SLICE-DCC and let the unit cool for several minutes. If problem persists, contact Vescent.

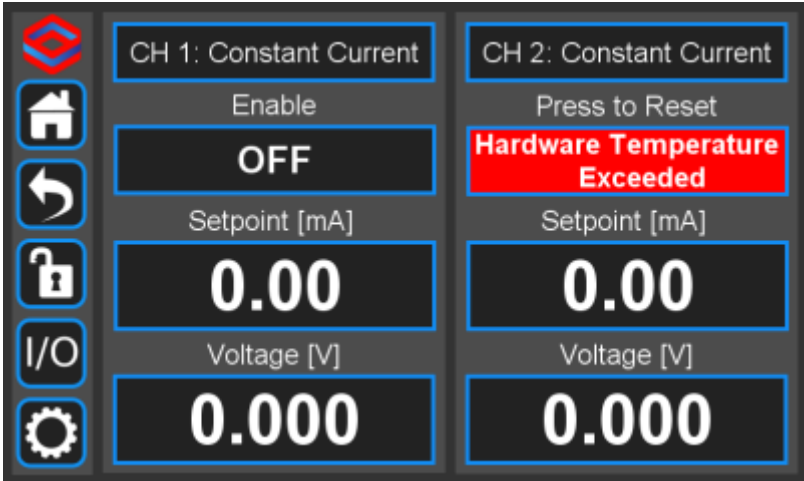


Fig. 41: Hardware Temperature Exceeded Error Message

Internal Case Temperature Exceeded

Dffects both channels and is displayed when the temperature inside the case exceeds a safe limit. Turn off the SLICE-DCC and let the unit cool for several minutes. If problem persists, contact Vescent.

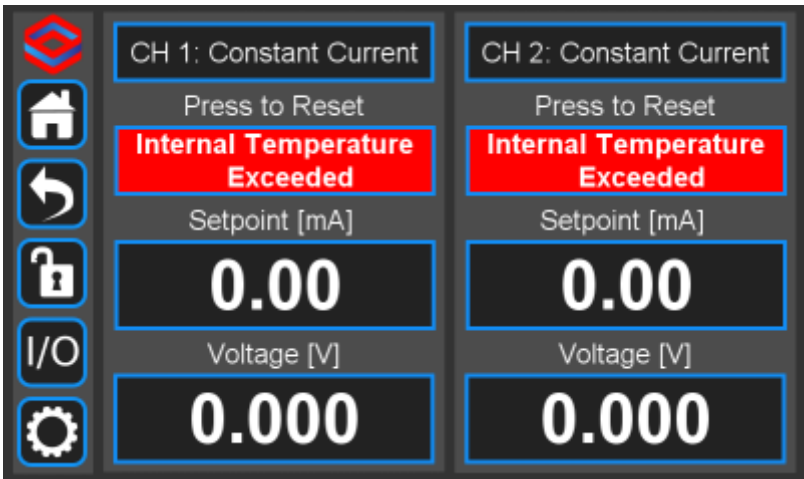


Fig. 41: Internal Temperature Exceeded Error Message

Interlock

Displayed on both channels when the interlock circuit is open. Double check that the Interlock Key is inserted and in the “Closed” position, and that the Interlock BNC port is connected to either an

interlock system, or the 50Ω terminator cap. Alternatively, if the Interlock BNC port is grounded, the Interlock warning may engage.

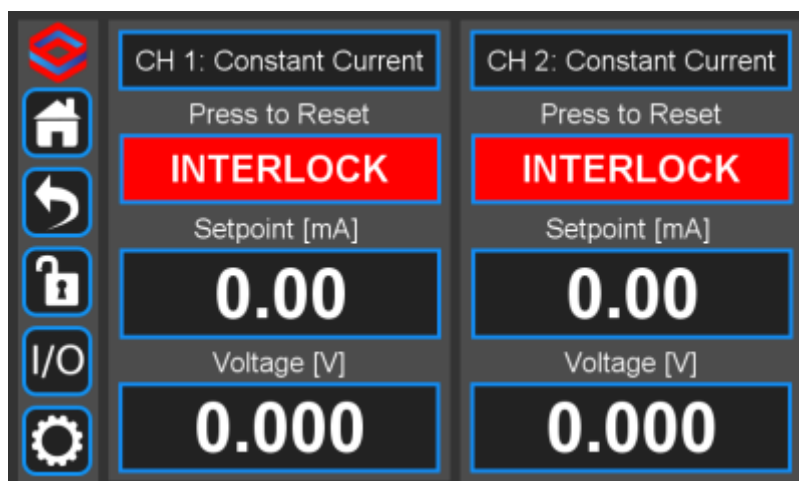


Fig. 43: Output Interlock Error Message

Open Circuit Over Voltage

Displayed on a channel that is started without a load attached. Double check connections on both the SLICE-DCC and the attached load. If problem persists, contact Vescent.

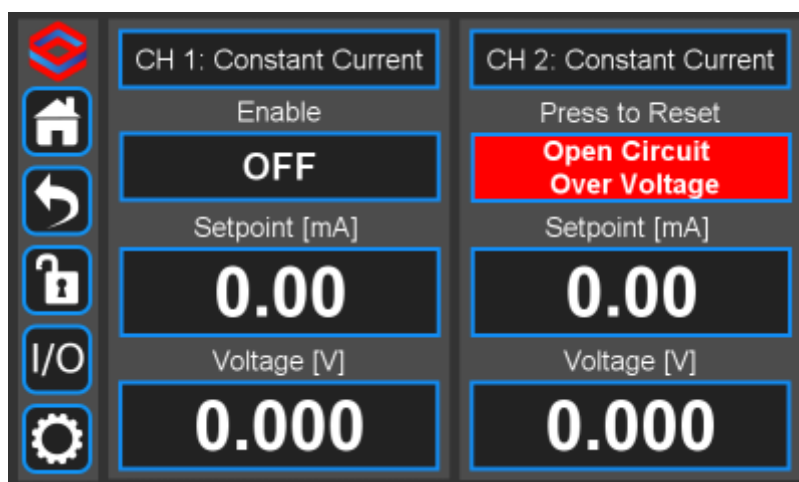


Fig. 41: Open Circuit Error Message

Possible Fault Detected

Displayed when current is being output in spite of the channel being disabled. The appearance of this fault indicates a potential hardware failure. Do **NOT** continue to use unit, and contact Vescent immediately.

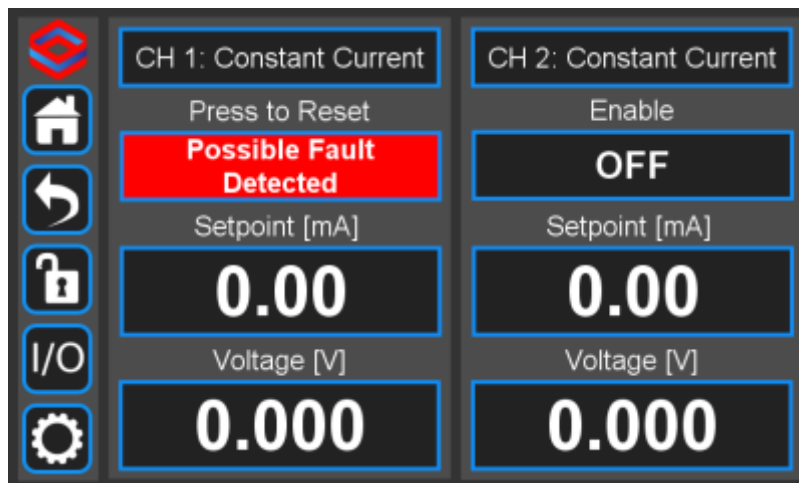


Fig. 41: Possible Fault Error Message

1)

Located in power receptacle on rear panel

2)

Subject to change without notice

3)

Constant Current Mode

4)

rms 100 Hz to 1 MHz

5)

-3 dB point

6)

front & rear modulation input ports

7)

constant power mode

8)

relative to maximum power

9)

See [table 3](#) for acceptable input ranges

10)

https://en.wikipedia.org/wiki/Logic_level

From:

<http://localhost:8800/> - **Product Manuals**

Permanent link:

<http://localhost:8800/doku.php?id=slice:dcc>

Last update: **2025/07/01 01:05**

